

Are your MRI contrast agents cost-effective?

Learn more about generic Gadolinium-Based Contrast Agents.



FRESENIUS
KABI

caring for life

AJNR

Reproducibility of the Whole-Brain *N*-Acetylaspartate Level across Institutions, MR Scanners, and Field Strengths

B. Benedetti, D.J. Rigotti, S. Liu, M. Filippi, R.I. Grossman and O. Gonen

This information is current as of April 20, 2024.

AJNR Am J Neuroradiol 2007, 28 (1) 72-75
<http://www.ajnr.org/content/28/1/72>

**ORIGINAL
RESEARCH**

B. Benedetti
D.J. Rigotti
S. Liu
M. Filippi
R.I. Grossman
O. Gonen

Reproducibility of the Whole-Brain *N*-Acetylaspartate Level across Institutions, MR Scanners, and Field Strengths

BACKGROUND AND PURPOSE: Radiologic markers in multicenter trials are often confounded by different instrumentation used. Our goal was to estimate the variance of the global concentration of the neuronal cell marker *N*-acetylaspartate (NAA) among research centers using MR imaging scanners of different models, from different manufacturers, and of different magnetic field strength.

MATERIALS AND METHODS: Absolute millimolar amounts of whole-brain NAA (WBNA) were quantified with nonlocalizing proton MR spectroscopy in the brains of 101 healthy subjects (53 women, 48 men) aged 16–59 years (mean, 34.2 years). Twenty-three were scanned at 1 institute in a 1.5T Siemens Vision; 31 from another institute were studied with a 1.5T Siemens SP63; 36 were scanned at a third institute (24 with a 1.5T Vision, 12 with a 3T Siemens Trio); and 11 were obtained at a fourth institute using a 4T GE Signa 5.x. The NAA amounts were quantified with phantom-replacement and divided by the brain volume, segmented from MR imaging, to yield the concentration, a metric independent of brain size suitable for cross-sectional comparison.

RESULTS: The average WBNA concentration among institutions was 12.2 ± 1.2 mmol/L. The subjects' WBNA distributions did not differ significantly ($p > .237$) among the 4 centers, regardless of scanner manufacturer, model, or field strength and irrespective of whether adjustments were made for age or sex.

CONCLUSION: Absolute quantification against a standard makes the WBNA concentration insensitive to the MR hardware used to acquire it. This important attribute renders it a robust surrogate marker for multicenter neurologic trials.

Multicenter phase II clinical trials for neurologic disorders frequently rely on surrogate markers to provide outcome measures sooner and with many fewer patients than clinical assessments.^{1–4} Such surrogates are often clinical MR imaging metrics, because of their sensitivity to disease-related abnormalities and their changes over time.^{1,5} Still, despite its sensitivity, MR imaging is not specific to the nature or true extent of brain tissue damage.^{1,6} Therefore, quantitative MR techniques (such as volumetry, magnetization transfer [MT], diffusion-weighted functional imaging, and proton MR spectroscopy [¹H-MR spectroscopy]) are sometimes also used.^{7,8} Although they could all potentially complement MR imaging,^{5,9} their interscanner variability, which is critical to avoid confounds in the data-consolidating stage, has not yet been fully established.¹⁰

One of the most prominent candidates for a neurologic surrogate marker is the amino acid derivative *N*-acetylaspartate (NAA), the second most abundant amino acid in the mammalian brain.^{11–14} Almost exclusive to neurons and their processes,^{15–17} its level is considered to reflect their health and attenuation.¹³ Because NAA can be quantified noninvasively with ¹H-MR spectroscopy,¹² this “marker + technique” duo is ideally suited to probe the underlying biochemistry of neuro-

logic disorders,¹³ both as structural abnormalities and as MR-occult pathologies.¹²

Unfortunately, brain ¹H-MR spectroscopy so far employs either small (1–8 cm³, single voxel) or large (≤ 100 cm³) 2D volumes-of-interest (VOI) placed away from the skull to avoid lipid contamination, missing most of the cortex.¹⁸ These limited sizes account for less than 10% of the brain volume, at best.^{19–21} Because many neurologic disorders are diffuse, missing 90%–99% of the brain implies that the overall extent of neuronal damage is represented by NAA decline in the VOI.²² Interpretation of ¹H-MR spectroscopy is further complicated by longitudinal VOI repositioning errors and the use of MR imaging scanners of various makes, model, and field strengths.

Although the repositioning and partial coverage limitations have recently been overcome with nonlocalizing ¹H-MR spectroscopy quantification of the whole-brain NAA (WBNA) concentration,^{23–25} its sensitivity to instrumentation change has not yet been established. This issue is examined in the present article by comparing the distribution of WBNA from several research centers and using various imagers by 2 manufacturers operating at different magnetic field strengths.

Materials and Methods

Human Subjects and MR Scanners

Because healthy persons are presumed, by definition, to be as similar as biologically possible, separate cohorts can be conveniently studied at different institutions, as opposed to transporting (the same) patient group around. Therefore, 101 healthy subjects (53 women, 48 men) aged 16–59 years (mean, 34.2 years) were recruited as follows: 23 subjects aged 31.0 ± 1.5 years (mean \pm SD) were studied at the first institution using a 1.5T Siemens Vision (Siemens, Erlangen Ger-

Received January 28, 2006; accepted after revision March 14.

From the Department of Radiology (B.B., D.J.R., S.L., R.I.G., O.G.), New York University School of Medicine, New York, New York; and Neuroimaging Research Unit (B.B., M.F.), Department of Neurology, Scientific Institute and University, San Raffaele Hospital, Milan, Italy.

This work was supported by National Institutes of Health grants EB01015, NS0050520, and NS39135.

Address correspondence to Oded Gonen, PhD, Department of Radiology, New York University School of Medicine, 650 First Ave, 6th Floor, New York, NY 10016; e-mail: oded.gonen@med.nyu.edu

many). Thirty-one subjects aged 33.0 ± 9.5 years were studied at the second institution using a 1.5T Siemens SP63. Thirty-six subjects aged 34.0 ± 8.9 years were studied at the third institution, as follows: 24 in a 1.5T Vision scanner and 12 in a 3T Siemens Trio. Finally, 11 subjects aged 43 ± 15 years were imaged at the fourth institution in a 4T Signa 5.x (GE Medical Systems, Milwaukee, Wis). All gave written informed consent, and the study was approved by the respective Institutional Review Boards.

MR Imaging—Brain volume, V_B , Segmentation

Each subject's brain parenchymal volume, V_B , was obtained from high-resolution T1-weighted sagittal magnetization-prepared rapid gradient-echo (TE/TR/TI, 7.0/14.7/300 ms; 128 1.5-mm sections; matrix, 256×256 ; FOV, 210×210 -mm²). The images were segmented into tissue and CSF, as described previously,²⁶⁻²⁸ with only the parenchyma accounted for in V_B .

MR Spectroscopy—WBNAA quantification

The amount of WBNAA, Q_{NAA} , was measured in each institution by using their imager in its standard neuro-MR configuration with a transmit-receive head coil. In each case, shimming yielded consistent 12 ± 3 , 20 ± 5 , and 26 ± 7 Hz whole-head water linewidths at 1.5-, 3-, and 4T, respectively, followed by the same nonlocalizing TE/TI/TR = 0/970/10,000 ms WBNAA ¹H-MR spectroscopy sequence.²³ The sequence nulls the NAA signal intensity every second shot with inversion-recovery, whereas the lipids' signals, with their short T1, ~220 ms, are always thermal (at either the TR of 10 seconds, or the TI of 970 ms). Therefore, an add-subtract scheme destructively interferes with their signal intensity,²³ as shown in Fig 1. Absolute quantification was done against a reference 3-L sphere of 1.5×10^{-2} mol of NAA in water. Subject and reference NAA peaks, S_S and S_R , were integrated from the resultant spectrum, as shown in Fig 1, and Q_{NAA} was obtained as^{23,29}:

$$1) \quad Q_{NAA} = 1.5 \times 10^{-2} \cdot \frac{S_S}{S_R} \cdot \frac{V_S^{180^\circ}}{V_R^{180^\circ}} \text{ moles,}$$

where $V_R^{180^\circ}$ and $V_S^{180^\circ}$ are the transmitter voltages into 50 Ω for non-selective 1-ms 180° inversion pulses on the reference and subject, respectively, reflecting relative coil loading. Note that slight changes were made to the sequence, increase of the chemical shift selection water suppression bandwidth, and decrease in the 1331 interpulse delays,²³ proportional to the magnetic field strength.

To account for natural variations in human head sizes, each subject's Q_{NAA} was divided by their V_B to yield the concentration

$$2) \quad \text{WBNAA} = \frac{Q_{NAA}}{V_B} \text{ mM,}$$

which is independent of brain size and therefore suitable for cross-sectional comparison. The intrasubject and intersubject variability of this metric was shown previously to be better than $\pm 7\%$.^{18,23}

Statistics

Analysis of variance (ANOVA) was used to compare sites and field strengths with respect to WBNAA. In particular, the Tukey honestly significant difference (HSD) procedure (to correct for multiple comparisons) was used in the ANOVA framework to make all pairwise comparisons among sites and field strengths with respect to WBNAA while maintaining the experiment-wise type I error rate for the set of comparisons at or below the 5% level. The ANOVA used WBNAA as the dependent

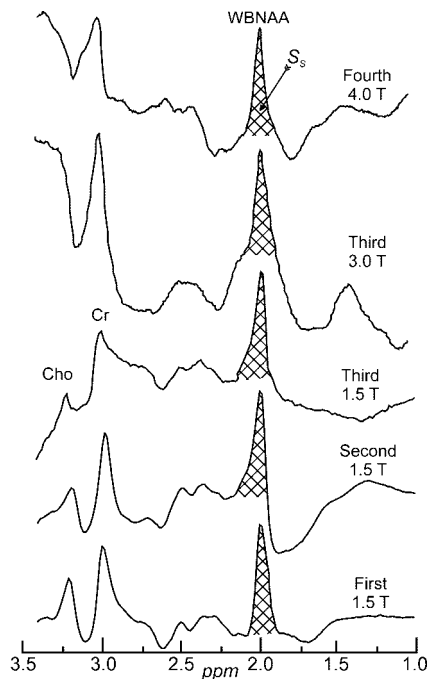


Fig 1. Sample whole-head ¹H-MR spectroscopy spectra from each of the MR imaging instruments used, with institution and field strength indicated. Although all the proton metabolites can be seen in the spectrum, note that because it was acquired in a whole-head, nonlocalized fashion, only the NAA peak is implicitly localized to the brain. The area of the NAA peak of the subject S_S , was integrated in each subject as shown and converted into absolute millimoles, Q_{NAA} , by comparing with the NAA peak area, S_R , in a reference phantom of known concentration as described by Eq. 1. Note the excellent signal-to-noise ratio of this short acquisition and the nearly total elimination of the skull's lipid signals from obscuring the spectrum.

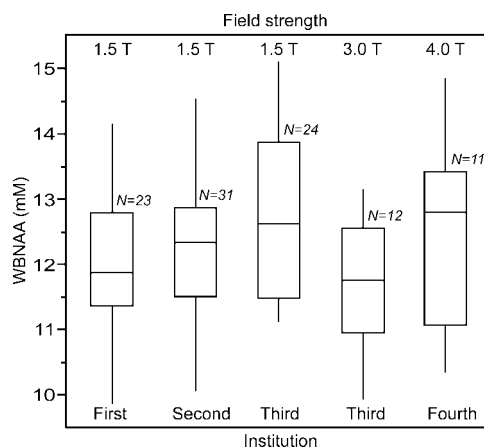


Fig 2. Box plot showing the 25%, 50% (median), and 75% quartiles (box) and $\pm 95\%$ (whiskers), of the distributions of the subjects' WBNAA concentrations in each of the 4 institutions, 5 scanners, 3 field strengths, and 2 manufacturers used in this study. Note that the differences among the distributions (means and SDs) are statistically insignificant, independent of the (healthy) subjects' age or sex, indicating that the methodology is robust to instrumentation differences.

variable and the model included subject age as a numeric factor and subject sex and either site or field strength as classification factors.

Results

The distribution of WBNAA values from each of the 5 scanners at the 4 centers are shown in Fig 2. There were no significant differences between them in terms of either the raw, unadjusted SDs or the SDs after adjustment for variation

Estimated mean \pm SD NAA concentrations at each institution.					
Institution	Subjects	Scanner Field, Manufacturer, Model	Mean WBNAA (mmol/L)	SD (Unadjusted) (mmol/L)	SD (adjusted)
First	$n = 23$	1.5 T, Siemens, Vision	11.7	1.3	1.3
Second	$n = 31$	1.5 T, Siemens, SP63	12.3	1.1	1.1
Third	$n = 24$	1.5 T, Siemens, Vision	12.6	1.2	1.2
	$n = 12$	3.0 T, Siemens, Trio	11.7	1.1	1.1
Fourth	$n = 11$	4.0 T, GE, Signa 5.x	12.8	1.5	1.5
Total	$n = 101$		12.2*	1.2*	1.2

Note:—WBNAA indicates whole-brain *N*-acetylaspartate. The SDs are presented as both unadjusted and adjusted with respect to confounding effects from age and gender (differences were in second decimal digit or smaller).

* Average of all subjects at all institutions.

attributable to age or sex ($p > .237$), as compiled in the Table. Furthermore, there were no significant differences between the mean WBNAA concentrations among the different instruments or research centers. Therefore, the invariant WBNAA concentration of healthy subjects is 12.2 ± 1.2 mmol/L.

Tukey HSD indicated that there were no significant differences ($p > .27$) between any pair of sites with respect to mean level of WBNAA. Furthermore, the same test has shown no significant difference between any 2 field strengths (HSD adjusted $p > .12$).

Discussion

Because of their exquisite sensitivity to brain abnormalities, MR-derived metrics are increasingly used as surrogates for efficacy in clinical trials of treatments for neurologic disorders.^{1,2,5,7-9,30} The problem, however, is that current clinical MR metrics do not fulfill some of the prerequisites needed to define a valid paraclinical surrogate.^{3,4} Key among these are that it be 1) simple to implement, 2) reproducible, 3) clinically meaningful, 4) pathologically specific, 5) sensitive to disease changes over time, and 6) of reasonably low labor intensity. The goals of this study were to determine the influence of center and hardware on WBNAA, an issue critical to the consideration of this technique for inclusion in multicenter clinical trials.

Prerequisite 1), above, is met by the WBNAA technique, as demonstrated by implementation in this study, across the multiple centers and scanners of different vintage, manufacturer, and magnetic field strength. These implementations also reflect, in a more subtle way, that the conjugate requirement 6), that of low labor intensity, is also met; ie, WBNAA acquisition and postprocessing are no more time-consuming than other quantitative MR imaging metrics. These 2 are “baseline” conditions for any technique to be considered for use in any multicenter trial.

Reproducibility, requirement 2) above, is also satisfied, as shown by Fig 2, as well as the statistical analyses in the Results, summarized in Table 1. Specifically, neither the 12.2 mmol/L average mean of the WBNAA distributions, nor its ± 1.2 mmol/L average SD, differs among imagers or centers. In other words, the variability of WBNAA across multiple imagers, $\pm 10\%$, is similar to that of any single instrument, assessed previously at $\pm 6\%$ – 7% in healthy control subjects.^{18,23} This finding is of particular importance if WBNAA is to be considered an adjunctive treatment efficacy measure for 2 main reasons: first, the scanners used represent many clinical research centers worldwide; second, most trials have treatment and control arms. Therefore, knowledge of the intrainstrument

and interinstrument variability in the control subjects will assist in determining the subject population required to detect a given expected treatment effect in the patients.

Previous studies have shown that the scan-rescan variability is a serious issue for quantities derived from conventional^{31,32} and MT MR imaging.³³ This has led to the formulation of rules standardizing acquisition across multiple centers, which suggested that upgrades or changes to scanners be limited during trials.^{9,31} This is a difficult rule to follow considering 1) the 2–3-year course of most clinical neurology trials versus the 5-year life span of modern MR scanners and 2) the manufacturers’ annual software upgrade cycles, some mandatory for regulatory compliance and others to keep the system current for its prime mission of clinical diagnostic MR imaging. The use of a calibration reference for the WBNAA measurement shows its potential to preempt *both* concerns.

The WBNAA method, however, is not without its limitations that need to be considered as part of a study design. Its main weakness is the total loss of localization. As a result, it is insensitive to changes smaller than 5%–6% (ie, oblivious to focal disorders [eg, stroke] and unable to discern between several foci of great loss and diffuse, overall smaller NAA decline). It also misses the NAA signal intensity from regions that suffer extreme susceptibility-driven field inhomogeneities (eg, the inferior frontal lobes, temporal lobes, and around the auditory canals). This loss, however, has been quantified previously at less than 10%.²⁵

In conclusion, this study indicates that the use of different MR scanners should not be considered a source of confounding variability for use of WBNAA in multicenter studies of neurologic disorders. Using it, therefore, allows the study designers to focus on the much more relevant criterion of patient accrual capability rather than hardware compatibility. The premise that this approach allows an overall assessment of neuroaxonal viability makes WBNAA an attractive surrogate marker for large-scale studies of treatment outcomes, especially for conditions characterized by diffuse or widespread brain damage, (eg, multiple sclerosis, AIDS, traumatic brain injury, Alzheimer disease, normal aging).

References

1. Miller DH, Grossman RI, Reingold SC, et al. **The role of magnetic resonance techniques in understanding and managing multiple sclerosis.** *Brain* 1998; 121:3–24
2. Arnold DL, Matthews PM. **MRI in the diagnosis and management of multiple sclerosis.** *Neurology* 2002;58:S23–31
3. Barkhof F, Held U, Simon JH, et al. **Predicting gadolinium enhancement status in MS patients eligible for randomized clinical trials.** *Neurology* 2005;65: 1447–54

4. Sormani MP, Bruzzi P, Comi G, et al. **The distribution of the magnetic resonance imaging response to glatiramer acetate in multiple sclerosis.** *Mult Scler* 2005;11:447–49
5. Sormani MP, Bruzzi P, Comi G, et al. **MRI metrics as surrogate markers for clinical relapse rate in relapsing-remitting MS patients.** *Neurology* 2002;58:417–21
6. Filippi M, Horsfield MA, Tofts PS, et al. **Quantitative assessment of MRI lesion load in monitoring the evolution of multiple sclerosis.** *Brain* 1995;118:1601–12
7. Rovaris M, Filippi M. **Magnetic resonance techniques to monitor disease evolution and treatment trial outcomes in multiple sclerosis.** *Curr Opin Neurol* 1999;12:337–44
8. Filippi M. **In-vivo tissue characterization of multiple sclerosis and other white matter diseases using magnetic resonance based techniques.** *J Neurol* 2001;248:1019–29
9. Filippi M, Dousset V, McFarland HF, et al. **Role of magnetic resonance imaging in the diagnosis and monitoring of multiple sclerosis: consensus report of the White Matter Study Group.** *J Magn Reson Imaging* 2002;15:499–504
10. Sormani MP, Iannucci G, Rocca MA, et al. **Reproducibility of magnetization transfer ratio histogram-derived measures of the brain in healthy volunteers.** *AJNR Am J Neuroradiol* 2000;21:133–36
11. Birken DL, Oldendorf WH. **N-acetyl-L-aspartic acid: a literature review of a compound prominent in 1H-NMR spectroscopic studies of brain.** *Neurosci Biobehav Rev* 1989;13:23–31
12. Danielsen EA, Ross B. *Magnetic Resonance Spectroscopy Diagnosis of Neurological Diseases.* New York: Marcel Dekker, Inc; 1999.
13. Arnold DL, de Stefano N, Matthews PM, et al. **N-Acetylaspartate: usefulness as an indicator of viable neuronal tissue** *Ann Neurol* 2001;50:823; discussion 824–25
14. Baslow MH. **Functions of N-acetyl-L-aspartate and N-acetyl-L-aspartylglutamate in the vertebrate brain: role in glial cell-specific signaling.** *J Neurochem* 2000;75:453–59
15. Simmons ML, Frondoza CG, Coyle JT. **Immunocytochemical localization of N-acetyl-aspartate with monoclonal antibodies** *Neuroscience* 1991;45:37–45
16. Moffett JR, Namboodiri MA, Cangro CB, et al. **Immunohistochemical localization of N-acetylaspartate in rat brain.** *Neuroreport* 1991;2:131–34
17. Jenkins BG, Klivenyi P, Kustermann E, et al. **Nonlinear decrease over time in N-acetyl aspartate levels in the absence of neuronal loss and increases in glutamine and glucose in transgenic Huntington's disease mice.** *J Neurochem* 2000;74:2108–19
18. Inglese M, Ge Y, Filippi M, et al. **Indirect evidence for early widespread gray matter involvement in relapsing-remitting multiple sclerosis.** *Neuroimage* 2004;21:1825–29
19. Brooks WM, Friedman SD, Stidley CA. **Reproducibility of 1H-MRS in vivo.** *Magn Reson Med* 1999;41:193–97
20. Marshall I, Wardlaw J, Cannon J, et al. **Reproducibility of metabolite peak areas in 1H MRS of brain.** *Magn Reson Imaging* 1996;14:281–92
21. Bokde AL, Teipel SJ, Zebuhr Y, et al. **A new rapid landmark-based regional MRI segmentation method of the brain.** *J Neurol Sci* 2002;194:35–40
22. De Stefano N, Narayanan S, Francis SJ, et al. **Diffuse axonal and tissue injury in patients with multiple sclerosis with low cerebral lesion load and no disability.** *Arch Neurol* 2002;59:1565–71
23. Gonen O, Viswanathan AK, Catalaa I, et al. **Total brain N-acetylaspartate concentration in normal, age-grouped females: quantitation with non-echo proton NMR spectroscopy.** *Magn Reson Med* 1998;40:684–89
24. Gonen O, Catalaa I, Babb JS, et al. **Total brain N-acetylaspartate: a new measure of disease load in MS.** *Neurology* 2000;54:15–19
25. Gonen O, Grossman RI. **The accuracy of whole brain N-acetylaspartate quantification.** *Magn Reson Imaging* 2000;18:1255–58
26. Udupa JK, Odhner D, Samarasekera S. **3DVIEWNIX: an open, transportable, multidimensional, multimodality, multiparametric imaging software system.** *Proc SPIE* 1994;2164:58–73
27. De Santi S, de Leon MJ, Rusinek H, et al. **Hippocampal formation glucose metabolism and volume losses in MCI and AD** *Neurobiol Aging* 2001;22:529–39
28. Smith SM, De Stefano N, Jenkinson M, et al. **Normalized accurate measurement of longitudinal brain change.** *J Comput Assist Tomogr* 2001;25:466–75
29. Soher BJ, van Zijl PC, Duyn JH, et al. **Quantitative proton MR spectroscopic imaging of the human brain** *Magn Reson Med* 1996;35:356–63
30. Filippi M, Horsfield MA, Ader HJ, et al. **Guidelines for using quantitative measures of brain magnetic resonance imaging abnormalities in monitoring the treatment of multiple sclerosis.** *Ann Neurol* 1998;43:499–506
31. Filippi M, van Waesberghe JH, Horsfield MA, et al. **Interscanner variation in brain MRI lesion load measurements in MS: implications for clinical trials.** *Neurology* 1997;49:371–77
32. Molyneux PD, Brex PA, Fogg C, et al. **The precision of T1 hypointense lesion volume quantification in multiple sclerosis treatment trials: a multicenter study.** *Mult Scler* 2000;6:237–40
33. Filippi M, Inglese M, Rovaris M, et al. **Magnetization transfer imaging to monitor the evolution of MS: a 1-year follow-up study.** *Neurology* 2000;55:940–46