

Are your MRI contrast agents cost-effective?

Learn more about generic Gadolinium-Based Contrast Agents.



**FRESENIUS
KABI**

caring for life

AJNR

MR imaging with topographic EEG electrodes in place.

R Lufkin, S Jordan, P Lylyck and F Vinuela

AJNR Am J Neuroradiol 1988, 9 (5) 953-954

<http://www.ajnr.org/content/9/5/953.citation>

This information is current as
of April 19, 2024.

MR Imaging with Topographic EEG Electrodes in Place

R. Lufkin,¹ S. Jordan,² P. Lylyck,¹ and F. Vinuela¹

Modern interventional neuroradiology procedures often require immediate feedback regarding the effects of induced alterations in cerebral blood flow. Although clinical feedback is helpful in many situations, there is an increasing reliance on real-time computed mapping of electroencephalographic data (CME). The procedures are also often done in stages with frequent interval feedback from other imaging studies, such as MR imaging, to assess brain parenchymal changes.

Unfortunately, the placement of the 30 or more scalp electrodes required for EEG monitoring is time-consuming and, once in place, these electrodes create severe image artifacts. We report here the use of nonferromagnetic EEG electrodes and wires that allow patients to be studied with MR imaging with the electrodes in place.

Materials and Methods

Patients referred for many neurointerventional procedures are first set up for computerized mapping of EEG. Thirty disk electrodes are applied with collodion according to the International 10–20 System with extra placements interpolated. The disks consist of gold-plated silver.* The wire leads are 1% cadmium, 99% copper alloy (copper

development #C16200) with silver plating.† Solder joints are made of pure tin [1].

Although the electrodes and wires were visible on the radiographs, they were acceptable for angiographic studies (Fig. 1). Extensive metal artifacts from the electrodes and wires, however, rendered the CT scanning nondiagnostic.

The MR examination was performed after the electrodes and wires were in place, but not during actual CME recording. Spin-echo pulse sequences were obtained by using a head coil on a 0.3-T whole body MR imager. No artifacts were visible on any of the pulse sequences chosen (Fig. 2)

Discussion

With increasing applications of MR imaging there has been a growing emphasis on selecting metals for use with MR that do not cause alterations in magnetic susceptibility. Abrupt local changes in induced magnetic field (susceptibility) result in magnetic-field inhomogeneities that interfere with the gradient fields used in imaging. The resulting local geometric distortions and alterations in image intensity can completely obscure underlying anatomy and pathology [2–5].

Through the use of either high-nickel-content stainless steel

Fig. 1.—Lateral postembolization scout view shows multiple CME electrodes in place.


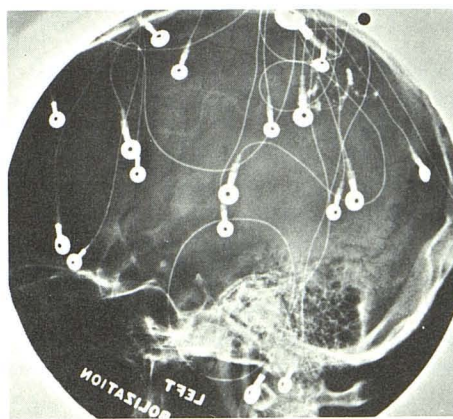


Fig. 2.—Coronal T1-weighted image (SE 500/28) of same patient with electrodes in place. Flow void is present in residual nidus of AVM (arrowhead). There is no evidence of artifact from the electrodes. Artifact was also absent on a T2-weighted image (SE 2000/84) (not shown).

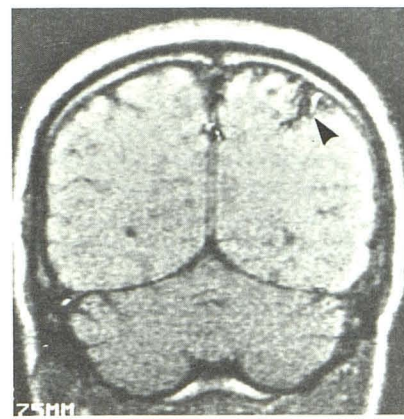

* Grass Co., Quincy, Mass., Pediatric Electrodes E-5-GH or Grass Adult E-6-GH.

† Grass Co., Quincy, Mass.

Received September 2, 1987; accepted after revision January 6, 1988.

¹ Department of Radiology, UCLA Medical Center, Los Angeles, CA 90024. Address reprint requests to R. B. Lufkin.

² Department of Neurology, UCLA Medical Center, Los Angeles, CA 90024.

alloys or nonferromagnetic metals, artifacts can be greatly diminished. Nickel reduces the ferromagnetic properties of the iron in the alloy by changing the highly susceptible form of alpha iron into less susceptible gamma iron. This decreases magnetic susceptibility differences between the alloy and surrounding tissues [4].

In this study we used silver-, gold-, and/or cadmium-based alloys, which are relatively nonferromagnetic for CME electrodes and wires. This preserves the high-performance properties of the recording electroencephalographic electrodes and connecting wires without producing significant artifacts on MR images. By using this design of wires we can now set up patients for continuous CME monitoring during staged angiographic or neurointerventional procedures with frequent MR follow-up examinations to assess parenchymal changes

in the brain without having to remove the electrodes at each MR examination.

REFERENCES

1. Newer MR, Jordan S, Ahn SS. Evaluation of stroke using frequency analysis and EEG mapping. *Neurology* **1987**;37:1153-1159
2. Lufkin R, Teresi L, Hanafey W. New needle for MR-guided biopsies. *AJR* **1987**;149:380-382
3. American Society for Metals. *Metals handbook*, vol. 3, 9th ed. Metals Park, Ohio: American Society for Metals, **1980**
4. New PFJ, Rosen BR, Brady TJ, et al. Potential hazards and artifacts of ferromagnetic and nonferromagnetic surgical and dental materials and devices in nuclear magnetic resonance imaging. *Radiology* **1983**;147:139-148
5. Ludeke KM, Roschmann P, Tischler R. Susceptibility artifacts in NMR imaging. *Magn Reson Imaging* **1985**;3:329-343