



## **Aneurysm Packing with HydroCoil Embolic System versus Platinum Coils: Initial Clinical Experience**

Harry J. Cloft and David F. Kallmes

*AJNR Am J Neuroradiol* 2004, 25 (1) 60-62

<http://www.ajnr.org/content/25/1/60>

This information is current as of August 4, 2024.

# Aneurysm Packing with HydroCoil Embolic System versus Platinum Coils: Initial Clinical Experience

Harry J. Cloft and David F. Kallmes

**Summary:** The HydroCoil Embolic System (HES; MicroVention, Aliso Viejo, CA) was developed to improve the efficacy of endovascular treatment of cerebral aneurysms. The HES may reduce recurrences of aneurysms by allowing for increased packing density as compared with platinum coils. We report our initial experience with the HES in the treatment of 11 patients with cerebral aneurysms and compare findings to those in size-matched control cases treated with platinum coils. The HES provided substantially improved volumetric packing of the aneurysm lumen relative to standard platinum coils (73% vs. 32%;  $P = .0001$ ).

A principal disadvantage of endovascular therapy of cerebral aneurysms with endovascular coils as compared with surgical clipping is aneurysm recurrence (1–3). Aneurysm recurrence following endovascular therapy is likely related, at least in part, to the density of packing of coils into the aneurysm, defined as volumetric percentage occlusion of the aneurysm cavity with the endovascular device (4–7). The HydroCoil Embolic System (HES; MicroVention, Aliso Viejo, CA) is designed with an expansile hydrogel that should theoretically fill more of the aneurysm lumen than standard platinum coils (8). We report our experience with the HES in 11 cases of cerebral aneurysms, with particular attention to the degree of aneurysm filling with embolic coils, and compare them to size-matched cases treated with platinum coils.

## Technique

The HES is constructed as a hybrid hydrogel-platinum coil device (Fig 1). The initial diameter of these devices is 0.009 inch, and the expanded diameter is 0.027 inch. In blood, the hydrogel swells to its maximum diameter (three times the original coil diameter) in approximately 20 minutes.

We chose to apply the HES to patients with “medium”-size aneurysms, ranging from 3.5 to 8.5 mm in diameter. The aneurysms treated with HES were treated in a standardized manner. A single, standard, platinum framing coil (MicroVention,

Aliso Viejo, CA; or Micrus Corporation, Mountain View, CA) was deposited in the aneurysm. HES coils (mean, 1.6 HES coils; range, 1–4 HES coils) were then deposited to fill most of the aneurysm volume. Finally, where indicated, the remainder of the aneurysm was then filled with small, soft platinum coils. Coils were added until no further coils would fit into the aneurysm without depositing in the parent vessel. Aneurysms included were located in wide variety of locations in both the anterior and posterior circulation.

A control group of 11 patients treated with standard platinum coils was assembled from our recent experience. These aneurysms were chosen to be similar in size to the aneurysms treated with HES and were located in a wide variety of locations in both the anterior and posterior circulation. These aneurysms were treated by adding coils until no further coils would fit into the aneurysm without depositing in the parent vessel.

None of cases required the use of balloon remodeling or adjunctive stent placement. Five patients in the HES group and four patients in the standard coil group had ruptured aneurysms. No clinical complications occurred in either the HES group or the standard coil group.

The aneurysm volume was calculated by assuming that the aneurysms were elliptical, by using the formula:

$$\text{Aneurysm volume} = 4 \pi (\text{height}/2 \times \text{length}/2 \times \text{width}/2)/3.$$

Coil volumes were calculated by the following formula:

$$\text{Coil volume} = \pi (\text{radius})^2 \times \text{length}.$$

The coil packing density was expressed by using the following formula:

$$\text{Packing density} = (\text{coil volume}/\text{aneurysm volume}) \times 100\%.$$

Aneurysm volumes, packing densities, numbers of coils per aneurysm, and number of coils per milliliter of aneurysm volume were compared between groups by using two-sample, two-tailed  $t$  tests (Table 1). The HES provided improved packing of the aneurysm lumen relative to standard platinum coils (72% vs. 32%;  $P = .0001$ ) (Fig 2). With HES, there were trends toward decreased coils per aneurysm (3.9 coils/aneurysm vs 4.6 coils/aneurysm) and decreased coils per milliliter of aneurysm volume (55 coils/mL versus 80 coils/mL), but these trends were not statistically significant.

## Discussion

Cerebral aneurysms treated with endovascular coil packing are only partially filled with coils, with most the intraluminal volume being filled initially with thrombus (9). Natural thrombolytic processes acting on this unstable thrombus may, in part, cause recurrence of aneurysms following endovascular coil therapy. An aneurysm filled with fewer coils and more thrombus could reasonably be expected to have a greater likelihood of recurrence. Indeed, low aneurysm coil packing density is associated with an increased risk of aneurysm recurrence, especially if less

Received June 4, 2003; accepted after revision July 13.

From the Department of Radiology, Mayo Clinic, Rochester, MN.

Drs. Cloft and Kallmes receive research support from MicroVention. Dr. Kallmes is also a stockholder in MicroVention.

Address correspondence to Harry J. Cloft, MD, PhD, Department of Radiology, Mayo Clinic, 200 First Street SW, Rochester, MN 55905.

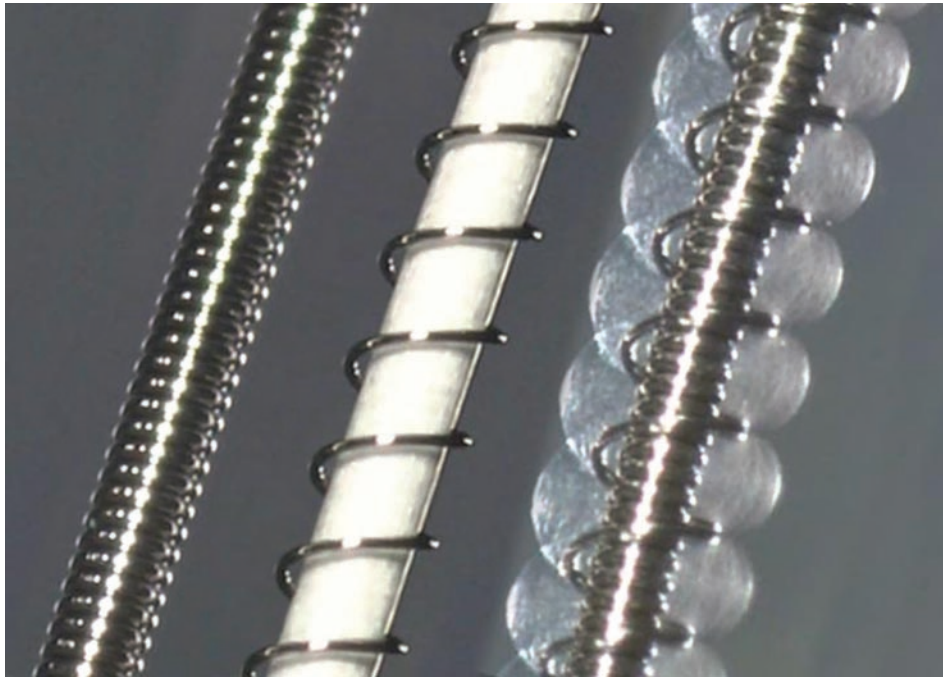


FIG 1. Hybrid hydrogel-platinum coil device. *Left*, Bare platinum coil. *Middle*, Prehydration image, showing initial profile of the device. Highly compact hydrogel material is wrapped around a platinum coil. An outer “overcoil” is wrapped around the hydrogel-covered coil. The outer diameter of the coil is 0.008 inch. The thickness of the hydrogel is approximately 0.0005 inch, such that the outer diameter of the gel covering is 0.009 inch. With the overcoil, the outer diameter is 0.013 inch. *Right*, Posthydration image of the device, showing marked expansion of the hydrogel material, which has become translucent. The radial thickness of the expanded hydrogel is approximately 0.009 inch, such that the total outer diameter of the hydrated device is 0.027 inch.

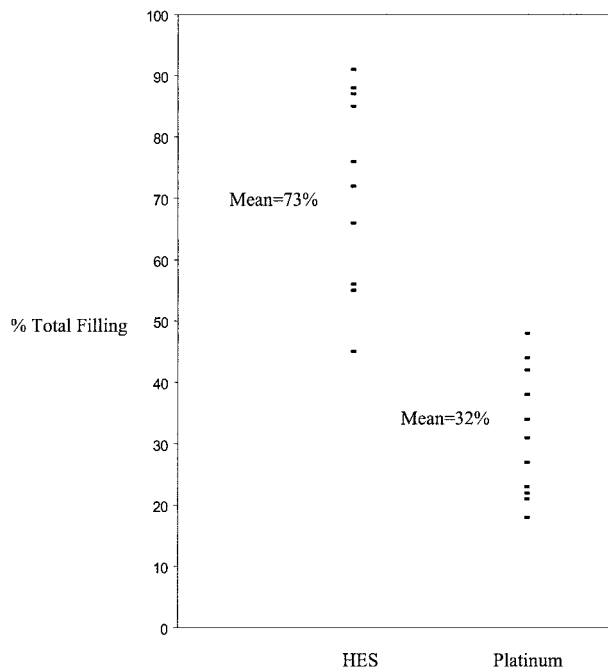


FIG 2. Scatter diagram of percent total occlusion of 11 aneurysms treated with platinum coils and 11 aneurysms treated with HES coils.

than 25% (4–7). The expanding hydrogel on the HES displaces clotting blood from the aneurysm lumen, resulting in a better packing density.

In our practice, we pack aneurysms tightly with

coils, stopping coil deposition only when no more coils can be safely deposited. Because of the volume of hydrogel deposited with the HES, we suspected that we might use fewer coils overall. There were trends toward decreases in coils per aneurysm and coils per milliliter of aneurysm volume, but these trends did not reach statistical significance. This trend toward use of fewer coils would probably be amplified in larger aneurysms. In addition, HES coils are now available in longer lengths and larger diameters than were previously available, which might also contribute to a trend toward use of fewer coils. Because the hydrogel is soft and deformable, it may not block the deposition of further platinum coils in the same way that a purely platinum coil does. HES coils are more expensive than standard platinum coils, but, because we tended to use only one or two in each case, we do not feel that they added substantial cost to the procedure.

We do not advocate using the HES coil as the only coil to treat an aneurysm. We used standard coils to form a “basket” or “framework” for subsequent deposition of HES coils. We then deposited HES coils to fill most the aneurysm volume. In six of 11 cases, we used only a single HES coil. Because of the expansion of the gel, HES coils have a maximum of 5 minutes of repositioning time before detachment or removal is necessary. We did not experience any deployment difficulty related to this time limitation. The HES coil is stiffer than standard coils, and therefore it is often not generally used as the final or “finishing” coil. Rather, the final coil was often a small, soft standard

TABLE 1: Comparison of aneurysms treated with adjunctive HydroCoil Embolization System (HES) vs. platinum coils alone

Patient	Aneurysm volume (ml)	% fill total	% fill HES	# HES coils	# platinum coils	#coils/aneurysm	# coils/ml
HES 1	0.063	66	41	1	3	4	63
HES 2	0.042	76	62	1	1	2	48
HES 3	0.029	87	63	1	2	3	103
HES 4	0.174	87	74	4	2	6	34
HES 5	0.063	91	71	2	1	3	48
HES 6	0.113	45	23	1	5	6	53
HES 7	0.094	55	27	1	3	4	43
HES 8	0.167	56	44	2	3	5	30
HES 9	0.092	72	56	2	3	5	54
HES 10	0.026	88	72	1	1	2	77
HES 11	0.059	85	76	2	1	3	51
Mean	0.084	73	55	1.6	2.3	3.9	55
Platinum 1	0.065	34			6	6	92
Platinum 2	0.042	44			7	7	167
Platinum 3	0.034	27			3	3	88
Platinum 4	0.031	48			5	5	161
Platinum 5	0.092	18			4	4	43
Platinum 6	0.079	42			4	4	51
Platinum 7	0.113	31			6	6	53
Platinum 8	0.236	23			4	4	17
Platinum 9	0.065	22			4	4	62
Platinum 10	0.079	21			5	5	63
Platinum 11	0.038	38			3	3	79
Mean	0.079	32			4.6	4.6	80
P value	.85	.0001				.23	.12

Note.—% fill total, percentage of aneurysm volume filled by embolic devices; % fill HES, percentage of aneurysm volume filled by HES coils; # coils/mL, number of coils per milliliter of aneurysm volume.

platinum coil. Smaller and softer HES coils suitable for use as “finishing” coils are currently under development.

This is a limited study of initial experience at a single center. Although we are encouraged by the improvement in aneurysm packing with HES, the effectiveness of hydrogel in preventing aneurysm recurrence remains to be proved. The HydroCoil for Embolic Aneurysm Occlusion (HEAL) trial is a multicenter trial that is currently underway that is expected to yield information regarding aneurysm recurrence following treatment with HES. We look forward to the HEAL trial results for proof that improved aneurysm packing with HES will yield a decrease in aneurysm recurrence.

### Conclusion

Our initial experience demonstrates that the HES allows substantially improved packing of the aneurysm lumen relative to standard platinum coils (72% vs. 32%;  $P = .0001$ ). We were able to significantly improve aneurysm packing even in cases in which only a single HES was used. Future, larger series with follow-up will be necessary to demonstrate that this improvement in aneurysm filling correlates with a decreased rate of aneurysm recurrence.

### References

- Cognard C, Weill A, Spelle L, et al. Long-term angiographic follow-up of 169 intracranial berry aneurysms occluded with detachable coils. *Radiology* 1999;212:348–356
- Debrun GM, Aletich VA, Kehrli P, et al. Selection of cerebral aneurysms for treatment using Guglielmi detachable coils: the preliminary University of Illinois at Chicago experience. *Neurosurgery* 1998;43:1281–1295
- Kuether TA, Nesbit GM, Barnwell SL. Clinical and angiographic outcomes, with treatment data, for patients with cerebral aneurysms treated with Guglielmi detachable coils: a single-center experience. *Neurosurgery* 1998;43:1016–1025
- Satoh K, Matsubara S, Hodoh H, Nagahiro S. Intracranial aneurysm embolization using interlocking detachable coils: correlation between volume embolization and coil compaction. *Intervent Neuroradiol* 1997;3:125–129
- Tamatani S, Ito Y, Abe H, et al. Evaluation of the stability of aneurysms after embolization using detachable coils: correlation between stability of aneurysms and embolized volume of aneurysms. *AJNR Am J Neuroradiol* 2002;23:762–767
- Uchiyama N, Kida S, Nomura M, et al. Significance of volume embolization ratio as a predictor of recanalization on endovascular treatment of cerebral aneurysms treated with Guglielmi Detachable Coils. *Intervent Neuroradiol* 2000;6:59–63
- Kawanabe Y, Sadato A, Taki W, Hashimoto N. Endovascular occlusion of intracranial aneurysms with Guglielmi detachable coils: correlation between coil packing density and coil compaction. *Acta Neurochir (Wien)* 2001;143:451–455
- Kallmes DF, Fujiwara NH. New expandable hydrogel-platinum coil hybrid device for aneurysm embolization. *AJNR Am J Neuroradiol* 2002;23:1580–1588
- Gruber A, Killer M, Bavinszki G, Richling B. Clinical and angiographic results of endosaccular coiling treatment of giant and very large intracranial aneurysms: a 7-year, single-center experience. *Neurosurgery* 1999;45:793–803